

# Bio-Avance

## Diode Module and Driver

### Replacement Parts 1-888-621-4484

- Laser Eyewear**
  - Eyewear # D-213-4600 Each \$29.95
- Laser Handpiece Replacement**
  - Laser Module # D-213-6700 Each \$699.95
  - Carbon Dye 200ml
- Carbon Dye # P-213-2500 Each \$49.95
- Laser Tattoo Post Treatment Gel 50ml
  - Stock # P-216-2500 Each \$49.99
- Laser Capillary Post Treatment Gel 50ml
  - Stock # P-216-2600 Each \$19.99
- Laser Post Treatment Aloe 50ml
  - Stock # P-216-2700 Each \$29.99
- TCA Enhanced Coupling Gel 50ml
  - Stock # P-216-2606 Each \$29.99
- Dermal Plast Topical Desensitizing Spray 50ml
  - Stock # P-216-2606 Each \$29.99

Prices are subject to change without notification. To order on-line, go to <http://www.centre-biotechnique-avance.com>  
For technical assistance beyond what this manual provides, please e-mail [customer\\_support@centre-biotechnique-avance.com](mailto:customer_support@centre-biotechnique-avance.com)  
Please allow 24 hours for processing.

**This Bio-Avance SDL produces laser radiation which can be harmful to the eyes. Always wear protective eye-wear while operating this equipment. Laser radiation has the capability to burn the skin if the technician does not closely observe the patient's reaction to the procedure. Laser and electrolysis procedures result in destruction of hair follicles and is irreversible. Always plan ahead before undertaking detail work such as eyebrow shaping or hairline contouring. Patch test a small area (no larger than 1X1 inch square) before full application. Allow 24 hours to determine the patient's reaction before applying full treatment.**

## Bio-Avance SDL80

Instruction Material for SDL  
Laser Nail Fungus and Hair Reduction System.

### Quick Setup Guide

Also approved for: Acne, Scars/Stretchmarks, Wrinkle Reduction, Photo Rejuvenation, Toning/Tightening and Hyper-pigmentation issues.



Keep this manual in a convenient place for quick and easy reference at all times.

In the interest of providing superior equipment, Bio Avance Industries reserves the right to modify or amend equipment specifications without notice or obligation.

2020 Bio-Avance Industries Ltd.

## Laser Hair Removal

There are currently two standard variations for the permanent removal of unwanted hair by way of laser radiation. The first of which being referred to as laser 'shaving'. The second is 'deep tissue traumatization' which targets living melanocytes or carbon dye in the follicle organ.

Laser shaving has the distinct advantage of showing immediate cosmetic improvement. A patient may walk into a laser hair removal office covered with unwanted hair then leave hairless and smooth a few hours later. Unfortunately for the patient (who may have spent \$1,000 or more for the visit) as much as 80% of their hair may return in about 6 weeks. Progressive permanency has been established at about 5-10% per treatment with the marginally inefficient 'laser shaving' method. The average investment of treatments (quantitatively) is 10-12 applications before hair growth is permanently halted (providing they are a good candidate for the procedure, see below).

The limitations for achieving permanent results in a prompt and expedient manner by way of laser shaving are many. Most of the laser radiation is absorbed and blocked by the hair above the skin. The fraction left over will be reflected and absorbed by the skin itself (especially in cases where the patient has high levels of pigment in the dermis). As little as 10% of the original photon output reaches the papilla matrix to produce thermal damage to the live hair follicle itself.

Laser shaving procedures are covered in this instruction booklet and may be used for those patients who prefer that particular method, however, for the purpose of efficacy and speed for permanent results this manual will focus primarily on the deep tissue traumatization method.

With the deep tissue method, a full 90% of the laser energy is passed through the epidermis (no reaction takes place on or above the surface of the skin) and as much as 98% passes with the use of a topical translucency enhancement gel. Only 2-5% loss of energy per mm of tissue depth occurs, which leaves very high levels of laser radiation at the precise areas to create thermal damage to the follicle. The deep tissue method requires that the hair be shaved prior to treatment. The hair below the skin will remain as a target for the laser energy.



A variation to this procedure requires the follicle organ to be removed from the skin by tweezing or waxing. The empty follicle is then treated with a carbon based dye. The advantages of this 'carbon dye' protocol are substantial. Melanin in human hair is not an efficient receptor for laser energy. Even black hair has only a 20-40% efficiency rating for the conversion of photon energy to heat. Carbon dye has a 99.997% heat exchange conversion ratio. This produces far greater thermal damage to the follicle itself. The next advantage to the carbon dye method is that no hair debris (carbonized hair) is left in the skin. The 'burnt hair' is visible through the skin as a dark spot and is poorly absorbed by the immune system (sometimes taking months to disappear). This can create pimple-like protrusions and, in some cases, infections. The third advantage to using the empty follicle shaft/carbon dye protocol is that laser radiation will not react with blond, red or grey hair growth. There simply is not enough pigment to create heat. By using carbon dye, the entire process becomes controlled, highly efficient and predictable.

## Client Pre-Qualifications


The best candidate for laser hair removal has fair skin with dark terminal hairs. Skin typing for exposure to ultraviolet light can be categorized by the Fitzpatrick classification, developed by Dr. Thomas Fitzpatrick of Harvard Medical School.

- Skin Type I:** Never tans, always burns (extremely fair skin, blonde hair, blue/green eyes)
- Skin Type II:** Occasionally tans, usually burns (fair skin, sandy to brown hair, green/brown eyes)
- Skin Type III:** Often tans, sometimes burns (medium skin, brown hair, brown eyes)
- Skin Type IV:** Always tan, never burns (olive skin, brown/black hair, dark brown/black eyes)
- Skin Type V:** Never burns (dark brown skin, black hair, black eyes)
- Skin Type VI:** (black skin, black hair, black eyes)

Types 1 through 4 are outstanding candidates. Type 5 will have excellent results as well, but care must be taken to assure that the laser will not burn the skin. Type 6 should not undergo laser hair removal unless used in conjunction with skin bleaching due to the high risk of burning and hypopigmentation issues.

**References:**  
 1. Bertram J, Carreras M, Egekvist H, Christensen K, Trullius A. Hair reduction using a new intense pulsed light radiator and a normal mode ruby laser. J Clin Laser Ther 2000; 2: 63-71.  
 2. Kaurer AM. Treatment of pseudofolliculitis with a pulsed infrared laser. Arch Dermatol 2000; 136:1343-6.  
 3. Erema S, Li C, Newman N. Laser hair removal with alexandrite versus diode laser using four treatment sessions: 1-year results. Dermatol Surg 2001; 27: 925-9.  
 4. Gupta M, Aslan G, Akoz T, Erdogan B. Comparison of alexandrite laser and electrolysis for hair removal. Dermatol Surg 2000; 26:37-41.  
 5. Benioni RJ, Lucit A, Galimberti M, Ferranti G. Long-term evaluation with long-pulsed redolium:YAG laser. Dermatol Surg 1999; 25:125-8.  
 6. Lloyd JK, Mikov N. Long-term evaluation of the long-pulsed alexandrite laser for the removal of bikini hair at structured treatment intervals. Dermatol Surg 2000; 26:633.

## SDL Laser Instrument

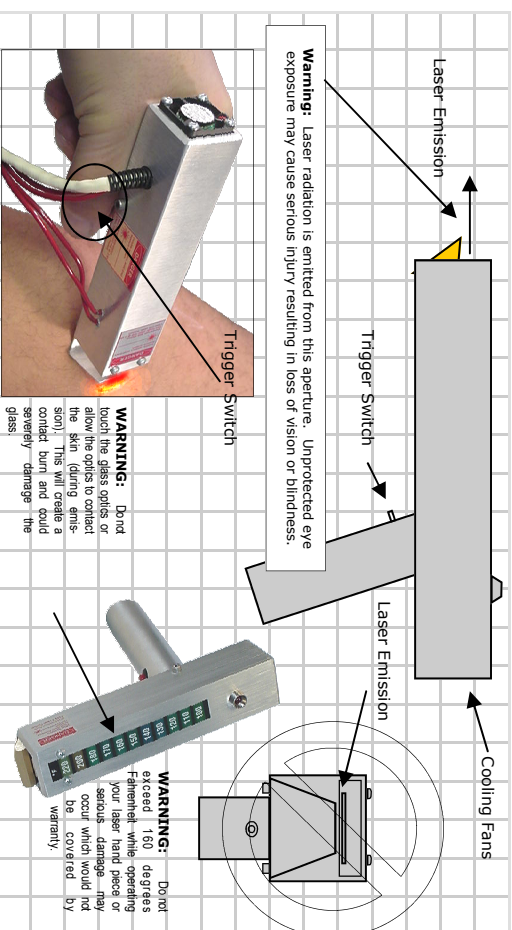


The SDL comes with a high output adjustable pulse frequency (fixed pulse duration) instrument for superior operator control. To prolong the life of your diode laser emitters it is advisable to activate the module in short bursts lasting no more than 1 second, while allowing an equal span of time of cooling between pulses. This will prevent overheating and potential damage to the laser crystals. The gallium arsenide laser diodes (emitters) are located inside the hand piece. Dropping or bumping the instrument may result in irreversible damage to the internal components and would not be covered by warranty. Pinching or bending the fiber optic leads that connect the instrument with the driver unit may also damage the laser.

**WARNING: Do not operate the laser on full power (Setting 3) and full pulse (Setting 3) for more than 1 second at a time. The diodes will overheat and may burn out. Failure to comply will void warranty.**

## Trouble Shooting

Should you encounter technical problems with your SDL Laser system, refer to the following guide for potential problems and their solutions.

- Unit is plugged into the wall, all accessories are correctly inserted into the unit but no laser output is being registered.
- ++Check all connections. Plug and unplug each one being sure all contacts are sound.
- ++Check all cords. Due to continual bending and fatigue, wires may fray or break resulting in full loss of power.
- ++Check Fuse: The unit has a fast-acting fuse mounted inside your unit to protect the delicate laser diode from voltage spikes, on-line power surges and electro-static discharge (ESD damage). Replace with 15 amp fast-acting type only. Failure to comply with these specifications may result in serious damage to your laser and will void all warranties.
- Unit clicks or makes noises.
- ++This clicking sound is normal. No service is required.
- Laser output is weak.
- ++Emitter output modules are blocked with carbonized debris (burnt hair etc.). Clean thoroughly with a cotton tipped applicator and alcohol. If the performance of the laser does not improve after cleaning the head your unit needs servicing by a qualified agent. Contact technical support for assistance.
- No output from the laser is registered after all trouble-shooting suggestions listed above have been checked.
- ++Probable diode failure. Unit needs servicing.

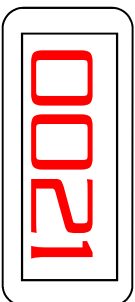

## Digital Pulse Counter

Specification	Min	Typ.	Max.	Unit	Reading/Second	Count
Accuracy	0.05	0.1	%(+1 count)		3	55
Linearity			+1	count	4	74
Sample rate	3			Samples/sec	5	92
Op. temp	0	50		°C	6	111
Temp. Stbl.	150			Ppm/°C	7	130

The meter may need recalibration by adjusting the on-board potentiometer. Two resistors, Ra and Rb may be used in order to alter the full scale reading (F.S.R.) of the meter. This counter contains a lithium ion battery and may explode if incinerated. Use proper disposal methods when discarding this device.

## Laser Startup Procedure

**Put on your laser eyewear before powering up your system. Wear the eye protection throughout the entire procedure.**

1. Turn the key lockout switch clockwise from 'neutral' to flashing red 'enabled' as shown.
2. Adjust the laser pulse to setting 1, 2 or 3. By pressing the trigger switch on the hand piece you will be delivering pulses of laser radiation. Adjust the pulse frequency to the desired level.
3. Set power level for treatment to intensity 3.
4. Use your pulse counter to accurately measure the total laser energy which is delivered to your client per treatment session. This counter can be reset by pressing the green button on the rear of your unit.

## Testing the Laser

With the power setting on 3, place the laser head 1/2 inch above the black test sheet included with your instruction material. Press the trigger switch in pulse mode for a brief duration (1 second or less). A series of red laser flashes will be evident which will ignite the test pad producing vapor and smoke. If no reaction occurs, check power setting and repeat.

**Note:** This laser operates at 808nm which is infrared (invisible to the human eye). Only a small amount of visible red is placed within the laser emitter for the purposes of alignment, focusing and ease of use. The DVD instructions sent with your laser machine show the laser as a bright white flashing during emission. This is simply due to the camera itself. Most digital cameras will pick up infrared energy and show it as brilliant white. Do not be concerned or confused. If your laser is burning the test sheet it is working correctly, despite the fact that your eyes cannot see the actual intensity.

If you have no laser test sheet you may use a clear balloon with a black marking pen. First inflate the balloon then make a round black mark the size of a quarter. When the laser beam strikes the black mark it will cause the balloon to burst. Should either of these tests result in poor performance of the laser your unit may be in need of service.






## Pulse Mode 3 and Diode Overheating

While using this laser in pulse mode on settings 1-2, there is little chance of overheating (which could lead to diode failure). However, using high power settings (#3) may lead to excessive heat build up. Short bursts of 1 second with a 1 second wait before the next emission are best on setting 3. Pushing the laser beyond the limits of performance will damage the gallium arsenide crystals, resulting in loss of intensity, performance, life expectancy of the laser which would not be covered by warranty.

The temperature strip on your SDL hand piece will turn black up to the correct number. It is important not to exceed 160 degrees Fahrenheit or damage may occur to your laser diode.

## Laser Head Maintenance

Clean the laser head and optics frequently. For light maintenance use acetone or alcohol on a cotton tip applicator. For more aggressive cleaning use an 'Exacto' to scrape any carbonized material from the laser head. Carbonized debris (residue from vaporized hair) can obstruct the laser treatment by occluding the optics (lens) as well as the articulating arm bracket.



**Always use caution when turning on and/or operating this system. The laser is very powerful and can cause serious eye or skin injury if used incorrectly.**

3

## Laser Resurfacing

Laser resurfacing is performed using a beam of laser energy which vaporizes the upper layers of damaged skin at specific and controlled levels of penetration. The procedure offers many advantages which others do not have. Unlike *Microneedling*, the laser penetrates deeply into the dermis where production of collagen proteins can be stimulated. Chemical peels can be very unpredictable and dangerous while lasers can be dialed in to deliver precisely the right amount of radiation to produce safe and effective results.



All resurfacing treatments work essentially the same way. First, the outer layers of damaged skin are stripped away. Then, as new cells form during the healing process, a smoother, tighter, younger-looking skin surface appears.

For superficial or medium resurfacing, the laser can be limited to the epidermis and papillary dermis. For deeper resurfacing, the upper levels of the reticular dermis can also be removed. Varied penetration allows treatment of specific spots or wrinkles.

For heavy resurfacing the use of carbon dye on the surface of the skin (also known as a 'carbon laser facial') will increase and amplify the laser's effect.

It's also important to consider the length of recovery when choosing among the skin-resurfacing alternatives. In general, the more aggressive the resurfacing procedure is, the more prolonged the recovery is likely to be. "Light" resurfacing procedures, such as superficial chemical peels or superficial laser resurfacing, offer shorter recovery times.

## General Dermatology

Treatment of additional skin afflictions such as Rosacea, Fine Wrinkles, Sun Damaged Skin, Acne Scars, Scars from CO2-laser resurfacing, Age Spots, Large Pores, Acne Prone Skin.


As the laser goes over the dermis, vascular spaces with hemoglobin in them absorb the laser energy thereby heating the surrounding tissue and stimulating the fibroblasts to produce type 1 collagen and dermal proteins. The treatment rearranges and/or replaces the solar elastosis in the upper dermis, resulting in NEW collagen formation.

What used to be loose, irregular collagen in the dermis is now tighter, refreshed and rejuvenated.

The benefits of each Diode Laser treatment over all other skin rejuvenation procedures include: Low downtime, non-surgical, little pain and discomfort, immediate results after 1 - 2 treatments, affordable, enhances your own collagen growth, produces more dermal proteins and treats all types of skin.


## Treatment Procedure: Resurfacing and Wrinkle Reduction

Deliver 1 second pulses of approximately 130 to 180 joules to each area of 1 cm square. Be very systematic and thorough, but resist the temptation to over treat. Applying more than 220 joules per cm2 may burn the skin.

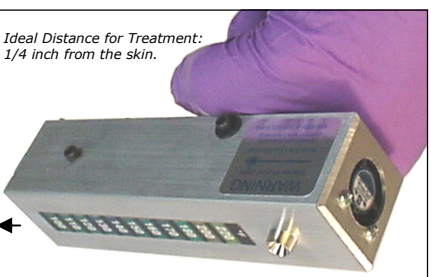

**Correct Hand Position for Treatments.**

Figure 1 shows normal sagging and wrinkling of the skin which can be expected as humans age. Figure 2 shows excellent improvement on a 47 year old female after 6 treatments.



Apply 'Laser Post Treatment Facial Gel' (see back page of pamphlet for ordering information). This formula contains aloe and glycolic acid, which produces a very mild chemical peel. Call your patient back in for a follow up in 48 hours. Additional treatments may be applied in 2-4 weeks depending on the level of dermal trauma the patient experience and their rate of healing.

8

## Nail Fungus Laser Treatment Procedure

Begin by having your client soak their feet for 20 minutes in warm water with antimicrobial soap. This will sterilize the feet and loosen the nail for carbon dye application. Dermatophytic onychomycosis (commonly called 'nail fungus') is **highly** contagious. It can be transmitted from toes to fingers and from client to practitioner. You must always wear gloves when touching infected tissue. Aggressively scrub the toes with a brush and clean the skin area (where onychomycosis is in high concentration from infected footwear and socks).




Using the special blunt ended syringe carefully slide the micro-tube under the nail as shown. Inject the carbon dye and saturate the area where the fungal infection is highest. It is not important for the dye to penetrate all areas as the laser itself will destroy the fungus in these hard to reach areas effectively. The use of carbon dye amplifies the laser heat and creates a much more effective thermal destruction of the fungus.



## Laser Application

Each 10mm square should be treated with seven pulses of high power laser energy. Use a grid layout as shown below. Areas that have ample carbon dye only require a single pulse. Areas without carbon dye should be treated with two to four pulses per mm squared. Each nail will require 60 to 90 seconds of Laser treatment. The time to do both feet (all ten nails) is approximately 5 to 10 minutes.

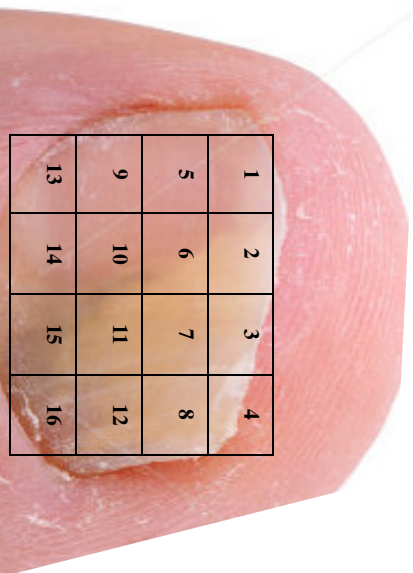

## Post Treatment Care

The use of an OTC anti fungal cream should be applied each day. Schedule the client for a follow up in 14 days. For complete destruction of the fungal infection, the entire nail must be allowed to completely grow out (pushing the diseased nail outward and allowing a healthy nail to replace it).

This procedure can take up to 6 months. Treating the client each 14 days is the best protocol as the technician can gauge the results. Each subsequent treatment session will require substantially less time as healthy nail overtakes the nail bed.

Client should discard all old footwear and socks. The virus lives in these materials and cannot easily be sanitized. The use of new footwear is the best way to avoid having the fungus return to the nail bed.

It is important to treat one tooth at a time, thoroughly. Each tooth will require 75-100 pulses which is about 20 seconds of actual laser exposure.


## Treatment Efficacy

Figures 1 and 2: Client before and after laser whitening. Gum health has also improved as the laser radiation kills microbes and bacteria in the tissue. Improvement will be noted after one treatment.



Additional treatments may be required to improve the shades. Client can expect to improve 3-5 shades per treatment.

## SDL Control Locations/Feature Descriptions

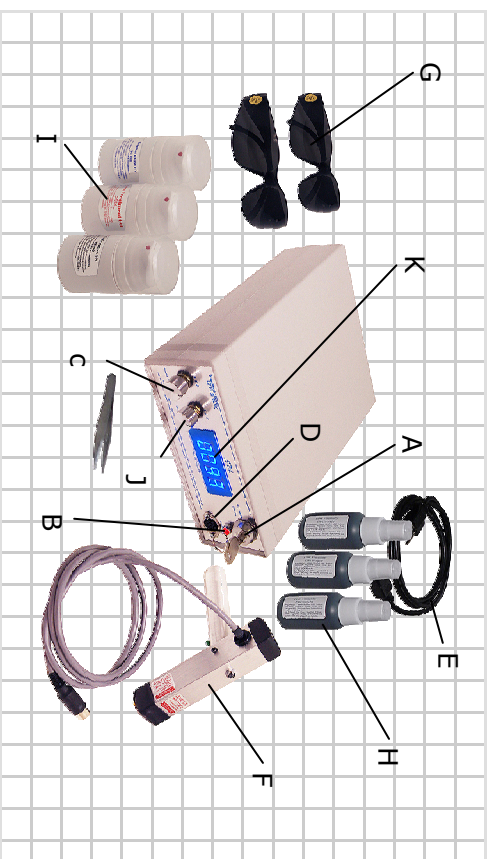

- A. **Key Lockout:** This feature is required by law on all high-power laser devices. The first step in the correct sequence to power-up your laser is to turn this lock clockwise using the special key included in your kit.
- B. **System Status LED:** This light will indicate system status (neutral or live). Green is neutral and red is live.
- C. **Pulse Control:** This allows the operator to set the number of laser pulses per second.
- D. **Laser Jack:** An eight-prong coaxial power jack for the diode laser hand piece.
- E. **Power Cord:** Rated for 60Hz, 120-240 V, 10 Amp with corresponding plug-style for country of destination.
- F. **Laser Instrument:** A 2cm single emitter high intensity pulsed laser with trigger switch.
- G. **Eyewear:** This is an essential part of the treatment process. Direct or reflective laser radiation can seriously injure the eye. Both the technician and the patient must use the protective eyewear while the laser is enabled or activated. Eyewear is intended for **accidental** exposure only. Never stare directly into a laser beam.
- H. **Carbon Dye:** This is an 'atomized' form of molecular carbon which easily penetrates deeply into the follicle shaft. The dye adds pigment which gives a receptor for the photon/heat exchange reaction. The carbon atoms will capture the laser energy and convert it into heat for the rapid and efficient cauterization of tissue for the permanent destruction of the hair follicle organ.
- I. **Gel Treatment Kit:** Dermal Plast desensitizing and Laser Post Treatment Gel for greater client comfort.
- J. **Intensity Dial:** Control feature for the regulated output of the laser module. Settings range from 1-3.
- K. **Pulse Counter:** Panel-mount digital display showing number of actual laser pulses delivered to the client. May be re set to zero by pressing the green button located on the rear panel of the SDL driver unit.

Intensity Setting 3	Pulse Frequency 3 (7 pulses/sec)	220 $\mu\text{m}^2/\text{second}$
Intensity Setting 2	Pulse Frequency 3 (7 pulses/sec)	180 $\mu\text{m}^2/\text{second}$
Intensity Setting 1	Pulse Frequency 3 (7 pulses/sec)	120 $\mu\text{m}^2/\text{second}$
Intensity Setting 3	Pulse Frequency 2 (5 pulses/sec)	180 $\mu\text{m}^2/\text{second}$
Intensity Setting 2	Pulse Frequency 2 (5 pulses/sec)	120 $\mu\text{m}^2/\text{second}$
Intensity Setting 1	Pulse Frequency 2 (5 pulses/sec)	90 $\mu\text{m}^2/\text{second}$
Intensity Setting 3	Pulse Frequency 1 (3 pulses/sec)	120 $\mu\text{m}^2/\text{second}$
Intensity Setting 2	Pulse Frequency 1 (3 pulses/sec)	90 $\mu\text{m}^2/\text{second}$
Intensity Setting 1	Pulse Frequency 1 (3 pulses/sec)	60 $\mu\text{m}^2/\text{second}$

## Laser Tattoo Removal

To begin the process it will be necessary for you to scrub the skin over the tattoo with an abrasive applicator. This is will remove the outer layers of the epidermis which will allow for greater penetration of the laser radiation.

Using a depilatory wax or epilation paper, remove all hair from the tattoo area. Hair growth will block some of the laser radiation from entering the tattoo. Follicles in the skin of the tattoo will also be permanently damaged by the radiation which may not be desirable to your patient.

### The Treatment Procedure

Carefully power up your laser (see page 4). Dial in full intensity on high pulse frequency. Place the emitter side down 1/2 inch above the skin over of the tattoo.


Deliver 1/2 to 1 second pulses (approximately 130-180 joules) to each area of 1 cm square (depending on color). Be very systematic and thorough, but resist the temptation to over treat.



Applying more than 220 joules per cm<sup>2</sup> may severely burn the skin. Black ink can be successfully treated with 120 jcm<sup>2</sup>. Blue and green normally requires 180 jcm<sup>2</sup>, and red requires up to 220.

The example tattoo at right required 51 pulses of 1 second each for a total of 5,000 joules.

Apply the Dermal Plast gel to the tattoo and allow to dry. This is a very important step which should not be omitted. Although the gel does contain the desensitizing compound Lidocaine it will be quite common for the patient to feel some burning in the minutes and hours following the procedure. This is quite normal. If the patient requests extra relief, apply a cold pack as needed.

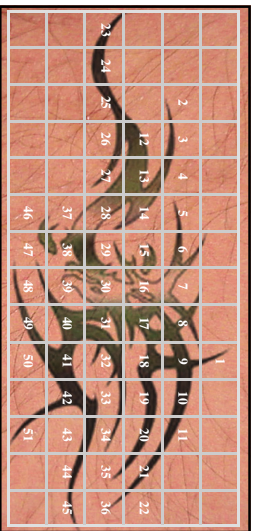

In picture number 5, you can see some of the redness, swelling and scabbing which may show up 1-3 days following treatment. In picture number 6 and 7, you can see some fading of the tattoo, but also a mild form of hypo pigmentation (loss of the patient's natural skin color). This condition is temporary and will subside as the melanin regenerates with natural healing. In picture number 7, you can see that the tattoo has faded to a point where it is not recognizable. This particular tattoo required 6 treatments over 7 months. It is always a good idea to take pictures of your patient's treatment areas to show them the steady improvement. This will help them to stay committed and motivated as the process requires a substantial investment of time.



Patient Group	Treatment Area	Tattoo Clearance (Average)	Notes
2 Patients Black Ink Only	Arms	99% after 3 mos.	5 treatment average
5 Patients Blue and Black Ink	Torso	99% after 3 - 12 mos.	8 treatment average

## Always Patch Test Your Client First

Before administering full treatment to any patient you must do a patch test. The best time is during their initial consultation. Apply 180jcm<sup>2</sup> to a single area (stationary exposure). To apply single pulses set your pulse frequency on 1 and pull the trigger switch once and release. If this test burns the patient (pain, distinct swelling and trauma to the skin will show) they are not suitable for laser epilation or laser procedures of any kind. This is generally a condition of persons who have black skin ( Fitzpatrick level 5 and 6).

### Treatment Variation 1: Deep Trauma on Shaved Hair



With this procedure, the hair is actually shaved by a razor prior to laser application. This leaves the follicle intact, which provides a target for the laser radiation. The skin must be thoroughly cleaned to allow for nearly 90-92% of the radiation to be sent deeply inside the tissue. If there is dirt, hair, or dead skin, the laser radiation may become blocked, thereby reducing the efficiency of the device.

Place the laser head over the skin as shown in figure 'a' (with the brass focal tip 1/2 inch above). **NOTE:** Never allow the laser optics lens to come in contact with the client's. Activate the laser on pulse setting 3 (7 pulses per second) while intensity is set at 3. Scan the treatment area at a rate of 1/2 inch per second at 180 jcm<sup>2</sup>.





### Laser Treatment Procedure 2: Laser Shaving

To shave the skin with a high power laser, trim the hair to 1/4 inch or so. If the hair is too long it will create debris which will block and obstruct the emission output resulting in loss of photon intensity. Should vaporized hair build up on the laser head, use ethyl alcohol on a cotton swab to clear.

Place the laser head above the skin as shown to the left in figures 'b' and 'c' and 'd'. The aluminum articulating tip may be in contact with the skin and the hand piece should be at a 85 degree angle to the surface so the optics do not contact the dermis. Activate the laser on pulse setting 3 (7 pulses per second) while intensity is set at 3. Scan the treatment area at a rate of 1/2 inch per second at 180jcm<sup>2</sup>. This procedure works well on coarse dark hair growth. Finer and lighter hair may not completely vaporize from the laser. In these cases, the use of carbon dye on the hair (or a dark hair dye) will improve the heat exchange reaction.

### Treatment Variation 3: Deep Trauma by Carbon Dye

Before applying treatment, remove all hair from the area by tweezing or waxing. Refer to pictures 1-5 below for proper technique for waxing and carbon dye application. Laser hair removal is most effective when applied to an empty follicle shaft. Human hair simply does not normally have enough pigment to allow for sufficient heat exchange to cauterize, desiccate and necrotize the cells which produce hair. To compensate for this lack of 'quantitative' and 'qualitative' photon targets, it will be necessary to place a high-density carbon dye inside the follicle prior to treatment.



Using a cotton-tipped applicator, completely cover the treatment area with the special dye included in your kit. Massage the dye into the follicle pore with a firm downward circular motion. Repeat 2-3 times to saturate the follicle pore. Use an **ethyl alcohol** based wipe to lightly clean the excess from the surface of the skin.

At this point you will have all desired follicles **visibly highlighted** with a dark spot (as seen above) and are ready to power up your laser for treatment. Place the laser head over the skin as shown in figure (with the focal arm touching the treatment area). Activate the laser on pulse setting 4 (7 pulses per second) while intensity is set at 3. Scan the treatment area at a rate of 1/2 inch per second.

## Treatment Efficacy for Permanent Hair Reduction

Permanent hair removal is a gradual process which takes 90 days or more for complete destruction of the follicle tissues. Each hair must go through its entire growth cycle for it to be effectively treated. Generally, it is only during the **early anagen** phase that it is vulnerable to destruction. The following chart will give you an accurate example of what the reduction in growth activity should look like from 30, 60 , and 90 days of treatments.



## Considerations for Safe Laser Hair Removal Treatment

**Treatment Around or Near the Eyes:** Great care must be exercised when working near the eyes. The laser emission is powerful enough to actually penetrate the eyelid and permanently damage the eye. Having the patient close their eyes is not satisfactory protection. The use of a dark-colored damp wash cloth which is folded over four times will deflect the harmful radiation; however, only laser protective eyewear is recommended.


**Treatment Around or Near Mucus Membranes:** Laser radiation will severely damage the tissues inside the nose and ear canal. Treatment should be avoided in these areas altogether.

**Treatment Around or Near the Genitals:** Laser hair removal is safe for application to the pubic regions including the reproductive organs of both sexes. Care must be taken into consideration in these areas due to the increased level of neural sensitivity. The patient may find the process uncomfortable without a topical desensitizing spray.


**Treatment Around or Near the Areola (nipple):** Laser hair removal is safe and effective on hair growth which occurs from the areola of both sexes.

**Post-Treatment:** The skin surrounding the treatment area will experience short-term erythema (reddening) which will subside within 12-24 hours.

Should the treatment area show signs of excess scabbing you may wish to reduce the overall treatment time or intensity. The application of a post-treatment cooling and healing gel (such as Aloe) is encouraged to speed healing and reduce sensitivity. Instruct the patient to refrain from applying cosmetics or sunbathing for at least 24 hours.



This laser can cause serious burns to the skin. All technicians should adopt the 'less is more' philosophy. It is far safer to have the patient come back for additional treatments than to administer too much radiation in one session resulting in tissue trauma and blistering.



<b>Emitted wavelength</b>	(808 ± 2) nm	<b>Classification:</b>	IV
<b>Output power</b>	User-adjustable 0 to 220 Joules	<b>Designation:</b>	QEP
<b>Generation modes</b>	LP/CW	<b>Manufacturer:</b>	Bio Advance
<b>Beam characteristic</b>	Semiconductor Diode	<b>Warranty:</b>	1 Year
<b>Pulse duration</b>	Manual Adjust	<b>Emission Indicator:</b>	Yes
<b>Weight</b>	15 kg max	<b>Key Lock:</b>	Yes
<b>Optics</b>	None	<b>Beam Shutter:</b>	No
<b>Dimensions</b>	170 x 500 x 370 mm	<b>ZICR# 1040, IEC 825-1:1993:</b>	No

Patient #	hair counts			12 week clearance percent
	pre	post	number of treatments	
1 Females, 2 males	274	9	12	97%
#1: laser shave procedure	327	19	8	94%
#2: deep tissue with hair	187	2	6	99%
#3: deep tissue with dye				

## Laser Tattoo Removal

Nearly 1/2 of all people with tattoos eventually want them removed. Until recently these people had no viable (and safe) options available to them. In the mid 1980's lasers had been used experimentally to remove the pigment with encouraging success rates. By the 90's they were producing very consistent and reliable results. Surprisingly, lasers do not actually burn the ink out; they fracture it into tiny pieces which are then removed from the skin by your immune system.

On average, professional tattoos require 5-6 treatments, while amateur tattoos may require 3-4 treatments, spaced approximately 2-4 weeks apart. The number of treatments depends on the amount and type of ink used and the depth of the ink in the skin. Occasionally technicians have needed to treat a tattoo 10-20 times.

**What should I charge for the procedure?** The fee depends on the size of each tattoo, and how many treatments it takes to lighten or remove it to your satisfaction. Each tattoo treatment generally costs \$135 for the 1st square inch and \$25 for each additional inch. If more than one tattoo is being treated at the same time, you may offer pricing alternatives. A consultation fee of \$40-\$60 should be assessed for this quote.

**What will the treatment be like?** It is less painful to have a tattoo removed than getting it put on. A numbing cream should be applied an hour or two before the procedure. After the procedure the treated area may blister, swell, crust, scab, or bleed slightly. Care for the treated area daily in order to prevent infection and to get the best possible healing results. The tattoo will then gradually fade for 2-4 weeks when it can be treated again. You may see additional fading for as long as several months so you can space the treatments farther apart but not closer than 2 weeks.


## Considerations for Safe Laser Tattoo Treatment

**Treatment on Skin with Hair Growth:** One of the major side effects of diode laser tattoo removal is destruction of hair follicles. If your client would like a tattoo removed from an area in which there is wanted hair growth, manually extract all follicles before treatment. The use of an aggressive depilatory wax is best. If the follicle is removed there will be far less damage to the papilla cells which produce growth. The hair follicle unit will regenerate in 4-6 weeks.

**Treatment Around or Near the Genitals:** Laser tattoo removal is safe for application to the pubic regions including the reproductive organs of both sexes. Care must be taken into consideration in these areas due to the increased level of neural sensitivity. The patient may find the process uncomfortable without a topical desensitizing spray.

**Treatment Around or Near the Eyes:** Great care must be exercised when working near the eyes. The laser emission is powerful enough to actually penetrate the eyelid and permanently damage the eye. Having the patient close their eyes is not satisfactory protection. The use of a dark-colored damp wash cloth which is folded over four times will deflect the harmful radiation; however, only laser protective eyewear is recommended.

**Post-Treatment:** The skin surrounding the treatment area may experience short-term erythema (reddening) which will subside within 12-24 hours. Should the treatment area show signs of excess scabbing you may wish to reduce the overall treatment time or intensity. The application of a post-treatment cooling and healing gel (such as Aloe) is encouraged to speed healing and reduce sensitivity. Instruct the patient to refrain from applying cosmetics or sunbathing for at least 24 hours.

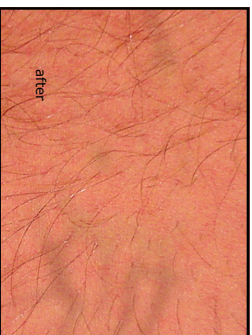

- Black Ink absorbs all wavelengths of light and responds very well to diode laser treatments.
- Green and Blue Ink absorbs 670-890nm light best and responds very well to diode laser treatments.
- Red, Orange, and Purple Inks absorb 500-700nm light best and will only show marginal improvement with diode laser treatments.
- Turquoise responds variably, depending on the pigments in the ink.
- Yellow tends to reflect light and does not respond well to diode laser treatments.